




## Validating Whole Slide Imaging (WSI) for Diagnostic Purposes in Pathology: Guideline Update

The 2021 evidence-based recommendations help pathologists and laboratories confirm diagnostic accuracy and equivalence of WSI systems with light microscopy (LM) before they are used for diagnostic purposes.

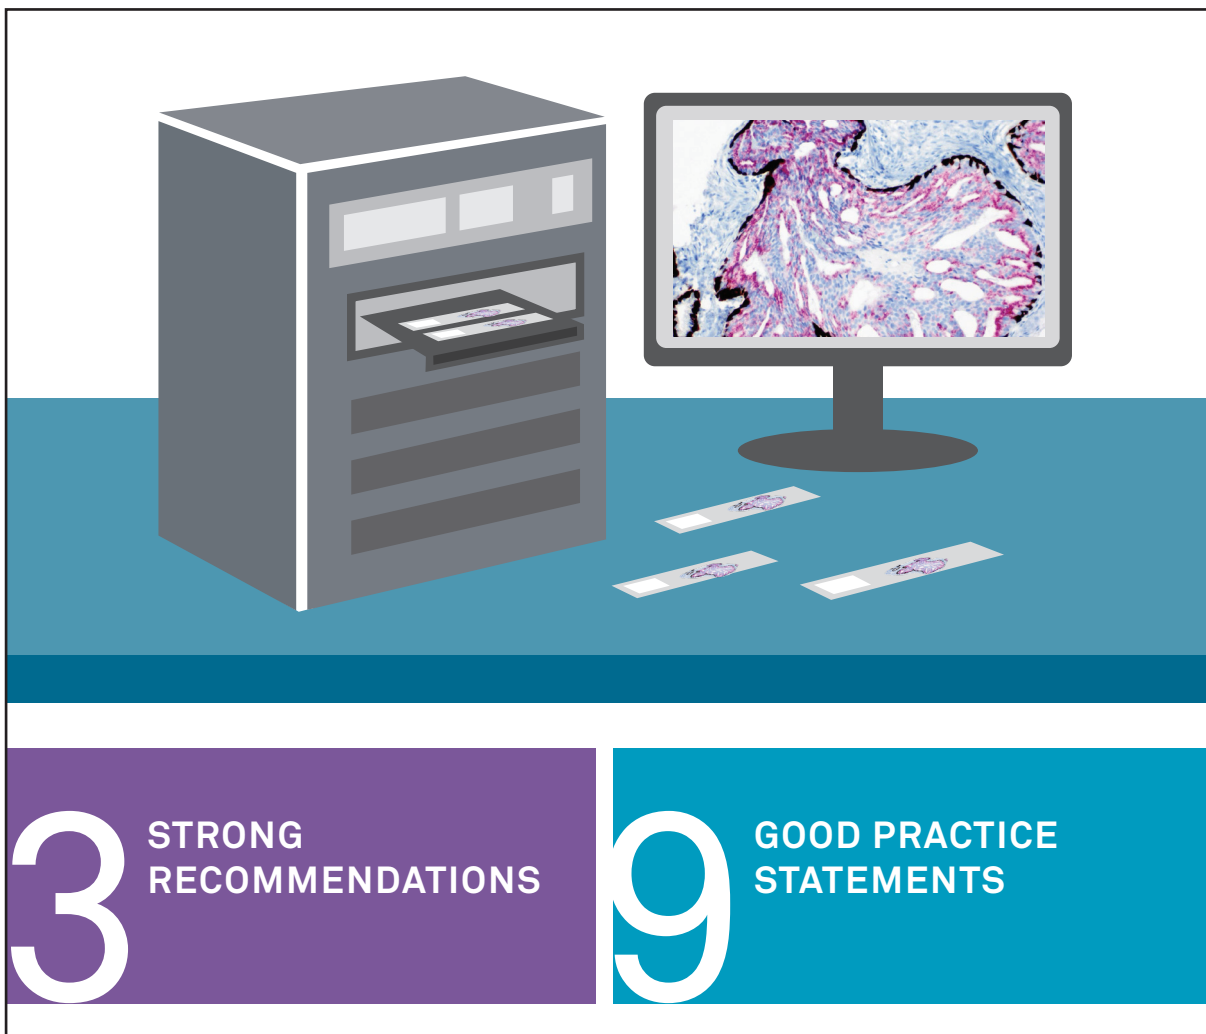

Evans A, Brown RW, Bui MM, et al. Validating whole slide imaging systems for diagnostic purposes in pathology: guideline update from the College of American Pathologists in collaboration with the American Society for Clinical Pathology and the Association for Pathology Informatics. *Arch Pathol Lab Med.* 2021;146(4):440-450. doi: 10.5858/arpa.2020-0723-CP